

Test Report

SL52025246081401TX

Date: June 08, 2020

Page 1 of 10

CONNEXIONS TECHNOLOGY (DONG GUAN) LTD
NO. 6, SHENBAO ROAD, QISHI TOWN, DONGGUAN CITY, GUANGDONG PROVINCE

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description : (A)Face mask

Style No. : CTPL-0020
 Composition : (A)Non-woven fabric, melt-blown fabric, hot air cotton
 Sample Color : (A)WHITE
 Manufacturer : CONNEXIONS TECHNOLOGY (DONG GUAN) LTD
 Country of Destination : Global
 Supplier : CONNEXIONS TECHNOLOGY (DONG GUAN) LTD

Test Performed : Selected test(s) as requested by applicant

Sample Receiving Date : Apr 28, 2020
 Testing Period : Apr 29, 2020 - Jun 08, 2020
 Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the sample(s) tested, for further details, please refer to the following page(s).

Conclusion:

| Sample No. | Recommendation Level |
|------------|----------------------|
| (A) | FFP2 NR |

Signed for and on behalf of
 SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center

Sara Guo (Account Executive)



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone: (86-788) 81871443, or email: CN.Goccheck@sgs.com

SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd
Testing Center, Pudong New Area, Shanghai, China

1 (86-21) 61402888 1 (86-21) 64966703 www.sgsgroup.com.cn
1 (86-21) 61402888 1 (86-21) 64966703 sgschina@sgs.com

Test Result

Respiratory Protective Devices — Filtering Half Masks to Protect against Particles — Requirements, Testing, Marking

(EN 149:2001+A1:2009)

Clause 7.4 Packaging

(EN 149:2001+A1:2009 Clause 8.2)

| Test Requirement | Results | Comment |
|--|---------|---------|
| Particle filtering half masks shall be offered for sale packaged in such a way that they are protected against mechanical damage and contamination before use. | Comply | Pass |

Clause 7.5 Material

(EN 149:2001+A1:2009, Clause 8.2 & 8.3.1 & 8.3.2)

| Test Requirement | Results | Comment |
|---|---------|---------|
| Materials used shall be suitable to withstand handling and wear over the period for which the particle filtering half mask is designed to be used. | Comply | Pass |
| After undergoing the conditioning described in 8.3.1 none of the particle filtering half masks shall have suffered mechanical failure of the facepiece or straps. | Comply | |
| When conditioned in accordance with 8.3.1 and 8.3.2 the particle filtering half mask shall not collapse. | Comply | |
| Any material from the filter media released by the air flow through the filter shall not constitute a hazard or nuisance for the wearer. | Comply | |

Clause 7.6 Cleaning and Disinfecting

(EN 149:2001+A1:2009, Clause 8.4 & 8.5 & 8.11)

| Test Requirement | Results | Comment |
|--|--|---------|
| If the particle filtering half mask is designed to be re-usable, the materials used shall withstand the cleaning and disinfecting agents and procedures to be specified by the manufacturer. With reference to 7.9.2, after cleaning and disinfecting the re-usable particle filtering half mask shall satisfy the penetration requirement of the relevant class. | Not applicable (Not designed to be re-usable) | N.A. |

Clause 7.7 Practical Performance

(EN 149:2001+A1:2009, Clause 8.4)

| Test Requirement | Results | Comment |
|---|------------------|---------|
| The particle filtering half mask shall undergo practical performance tests under realistic conditions. These general tests serve the purpose of checking the equipment for imperfections that cannot be determined by the tests described elsewhere in this standard. | No imperfections | Pass |

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone : (021-7881817144),
e-mail : CN.Goccheck@sgs.com



3 Building No.889, Yuhai Road, Xuhui District Shanghai, China: 200233
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233

1 (86-21) 61402888 1 (86-21) 64966703 www.sgsgroup.com.cn
1 (86-21) 61402888 1 (86-21) 64966703 sgschina@sgs.com

Clause 7.8 Finish of Parts

(EN 149:2001+A1:2009, Clause 8.2)

| Test Requirement | Results | Comment |
|---|-------------------------|---------|
| Parts of the device likely to come into contact with the wearer shall have no sharp edges or burrs. | No sharp edges or burrs | Pass |

Clause 7.9.1 Total Inward Leakage

(EN 149:2001+A1:2009, Clause 8.5)

| Test Requirement | Results | Comment |
|--|----------------------------|-------------------------|
| The total inward leakage consists of three components: face seal leakage, exhalation valve leakage(if exhalation valve fitted) and filter penetration. For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than: 25% for FFP1, 11% for FFP2, 5% for FFP3 and, in addition, at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than: 22% for FFP1, 8% for FFP2, 2% for FFP3 | Detail refer to Appendix 1 | Meet FFP1, Meet FFP2 |

Appendix 1: Summarization of Test Data**Inward Leakage Test Data**

| Subject | Sample No. | Condition | Walk(%) | Head Side/side(%) | Head up/down(%) | Talk(%) | Walk(%) | Mean(%) |
|---------|------------|-----------|---------|-------------------|-----------------|---------|---------|---------|
| Zhou | 1 | A.R. | 6.11 | 5.08 | 7.73 | 5.47 | 6.33 | 6.14 |
| Luo | 2 | A.R. | 7.84 | 6.74 | 7.17 | 5.90 | 8.26 | 7.18 |
| Lu | 3 | A.R. | 6.44 | 4.86 | 6.48 | 6.18 | 7.10 | 6.21 |
| Wang | 4 | A.R. | 5.86 | 5.60 | 4.78 | 5.41 | 4.82 | 5.29 |
| Bao | 5 | A.R. | 8.29 | 8.66 | 7.51 | 6.82 | 5.91 | 7.44 |
| Ding | 6 | T.C. | 5.59 | 4.76 | 5.54 | 4.97 | 5.85 | 5.34 |
| Li | 7 | T.C. | 8.25 | 7.75 | 6.81 | 7.63 | 8.40 | 7.77 |
| Chen | 8 | T.C. | 5.45 | 5.05 | 5.98 | 5.58 | 5.35 | 5.48 |
| Song | 9 | T.C. | 5.60 | 6.81 | 5.64 | 6.70 | 6.99 | 6.35 |
| Ye | 10 | T.C. | 8.33 | 7.88 | 8.11 | 6.80 | 8.22 | 7.87 |

Facial Dimension(mm)

| Subject | Face length | Face Width | Face Depth | Mouth Width |
|---------|-------------|------------|------------|-------------|
| Chen | 125 | 150 | 120 | 58 |
| Lu | 115 | 132 | 107 | 48 |
| Zhou | 115 | 135 | 106 | 52 |
| Li | 125 | 130 | 107 | 46 |
| Luo | 125 | 136 | 100 | 43 |
| Zheng | 128 | 140 | 112 | 55 |
| Wang | 120 | 147 | 103 | 48 |
| Song | 120 | 140 | 100 | 50 |
| Bao | 130 | 134 | 104 | 50 |

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed elsewhere, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from observing all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone : (86-21) 61402888, e-mail : CH.Gocchiali@sgs.com



SGS Testing Center (Shanghai) Co., Ltd.
No.889 Yan'an Road, Xuhui District, Shanghai, China 200233

1 Building, No.889, Yan'an Road, Xuhui District, Shanghai, China 200233
中国·上海·徐汇区宜山路889号1号楼 邮编: 200233

1 (86-21) 61402888

1 (86-21) 64966703

www.sgsgroup.com

1 (86-21) 61402888

1 (86-21) 64966703

sgschina@sgs.com

| | | | | |
|------|-----|-----|-----|----|
| Ding | 134 | 150 | 110 | 52 |
| Liu | 120 | 135 | 117 | 50 |
| Ye | 126 | 137 | 105 | 52 |

Clause 7.9.2 Penetration of Filter Material

(EN 149:2001+A1:2009, Clause 8.11 & EN 13274-7:2019)

| Test Requirement | | | Results | Comment |
|---|--------------------------------------|-----------------------------------|----------------------------|-------------------------|
| The penetration of the filter of the particle filtering half mask shall meet the requirements of the following table. | | | | |
| Classification | Maximum penetration of test aerosol | | | |
| | Sodium chloride test 95 l/min % max. | Paraffin oil test 95 l/min % max. | | |
| FFP1 | 20 | 20 | Detail refer to Appendix 2 | Meet FFP1, Meet FFP2 |
| FFP2 | 6 | 6 | | |
| FFP3 | 1 | 1 | | |

Appendix 2: Summarization of Test DataPenetration of filter material

| Aerosol | Condition | Sample No. | Penetration (%) |
|----------------------|--|------------|-----------------|
| Sodium chloride test | As received | 1 | 0.117 |
| | | 2 | 0.126 |
| | | 3 | 0.119 |
| | Simulated wearing treatment | 4 | 0.145 |
| | | 5 | 0.190 |
| | | 6 | 0.175 |
| | Mechanical strength +Temperature conditioned | 7 | 0.412 |
| | | 8 | 0.317 |
| | | 9 | 0.396 |
| Paraffin oil test | As received | 10 | 0.201 |
| | | 11 | 0.306 |
| | | 12 | 0.287 |
| | Simulated wearing treatment | 13 | 0.279 |
| | | 14 | 0.314 |
| | | 15 | 0.336 |
| | Mechanical strength +Temperature conditioned | 16 | 3.674 |
| | | 17 | 4.124 |
| | | 18 | 4.176 |

Flow conditioning : Single filter: 95.0 L/min

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone: (021-78818171443),
or email: CN.Goccheck@sgs.com



SGS Testing Center (Shanghai) Co., Ltd.
Inspection & Testing Service

3 Building No.889, Yuhai Road, Xuhui District Shanghai, China: 200233
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233

1 (86-21) 61402888 1 (86-21) 64968703 www.sgsgroup.com.cn
1 (86-21) 61402888 1 (86-21) 64968703 sgschina@sgs.com

Clause 7.10 Compatibility with Skin

(EN 149:2001+A1:2009, Clause 8.4 & 8.5)

| Test Requirement | Results | Comment |
|--|---|---------|
| Materials that may come into contact with the wearer's skin shall not be known to be likely to cause irritation or any other adverse effect to health. | No irritation or any other adverse effect to health | Pass |

Clause 7.11 Flammability

(EN 149:2001+A1:2009, Clause 8.6)

| Test Requirement | Results | Comment |
|--|----------------------------|---------|
| The material used shall not present a danger for the wearer and shall not be of highly flammable nature When tested, the particle filtering half mask shall not burn or not to continue to burn for more than 5 s after removal from the flame. | Detail refer to Appendix 3 | Pass |

Appendix 3: Summarization of Test DataFlammability

| Condition | Sample No. | Result |
|-------------------------|------------|--------|
| As received | 1 | NIL |
| | 2 | NIL |
| Temperature conditioned | 3 | NIL |
| | 4 | NIL |

Clause 7.12 Carbon Dioxide Content of The Inhalation Air

(EN 149:2001+A1:2009, Clause 8.7)

| Test Requirement | Results | Comment |
|--|----------------------------|---------|
| The carbon dioxide content of the inhalation air (dead space) shall not exceed an average of 1,0 % (by volume) | Detail refer to Appendix 4 | Pass |

Appendix 4: Summarization of Test DataCarbon Dioxide Content of The Inhalation Air

| Condition | Sample No. | Result(%) | |
|-------------|------------|-----------|-----------------|
| As received | 1 | 0.4875 | Mean value:0.49 |
| | 2 | 0.4862 | |
| | 3 | 0.4869 | |

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone : (86-788) 81871443, or email: CN.Goccheck@sgs.com



1 Building, No.889, Yuhai Road, Xuhui District, Shanghai, China: 200233
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233
1 (86-21) 61402888 1 (86-21) 64966703 www.sgsgroup.com.cn
1 (86-21) 61402886 1 (86-21) 64966703 sgschina@sgs.com

Clause 7.13 Head Harness

(EN 149:2001+A1:2009, Clause 8.4 & 8.5)

| Test Requirement | Results | Comment |
|---|---------|---------|
| The head harness shall be designed so that the particle filtering half mask can be donned and removed easily. | Comply | Pass |
| The head harness shall be adjustable or self-adjusting and shall be sufficiently robust to hold the particle filtering half mask firmly in position and be capable of maintaining total inward leakage requirements for the device. | Comply | |

Clause 7.14 Field of Vision

(EN 149:2001+A1:2009, Clause 8.4)

| Test Requirement | Results | Comment |
|--|---------|---------|
| The field of vision is acceptable if determined so in practical performance tests. | Comply | Pass |

Clause 7.15 Exhalation Valve(s)

(EN 149:2001+A1:2009, Clause 8.2 & 8.9.1 & 8.3.4 & 8.8)

| Test Requirement | Results | Comment |
|---|---|---------|
| (a) A particle filtering half mask may have one or more exhalation valve(s), which shall function correctly in all orientations. | Not applicable due to No exhalation valve | N.A. |
| (b) If an exhalation valve is provided it shall be protected against or be resistant to dirt and mechanical damage and may be shrouded or may include any other device that may be necessary for the particle filtering half mask to comply with 7.9. | Not applicable due to No exhalation valve | |
| (c) Exhalation valve(s), if fitted, shall continue to operate correctly after a continuous exhalation flow of 300 l/min over a period of 30 s. | Not applicable due to No exhalation valve | |
| (d) When the exhalation valve housing is attached to the faceblank, it shall withstand axially a tensile force of 10N applied for 10 s. | Not applicable due to No exhalation valve | |

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone : (021-788) 81871443, or email: CN.Goccheck@sgs.com



3rd Building, No.889, Yuhai Road, Xuhui District, Shanghai, China: 200233
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233

T: (86-21) 61402888 F: (86-21) 64966703 www.sgsgroup.com.cn
E: sgschina@sgs.com

Clause 7.16 Breathing Resistance

(EN 149:2001+A1:2009, Clause 8.9)

| Test Requirement | | | | | | Results | | | Comment | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
|--|-------------------------------------|----------|-----------|------------|--|----------------------------|--|--|---------------------------------------|--|----------------|-------------------------------------|--|--|--|--|------------|--|--|------------|--|----------|----------|-----------|--|--|------|-----|-----|-----|--|--|------|-----|-----|-----|--|--|------|-----|-----|-----|--|--|
| The penetration of the filter of the particle filtering half mask shall meet the requirements of the following table. | | | | | | Detail refer to Appendix 5 | | | Meet FFP1, Meet FFP2, Meet FFP3 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th rowspan="3" style="width: 15%;">Classification</th> <th colspan="5" style="text-align: center; border-bottom: 1px solid black;">Maximum permitted resistance (mbar)</th> </tr> <tr> <th colspan="3" style="text-align: center;">Inhalation</th> <th colspan="2" style="text-align: center;">Exhalation</th> </tr> <tr> <th style="text-align: center;">30 l/min</th> <th style="text-align: center;">95 l/min</th> <th style="text-align: center;">160 l/min</th> <th colspan="2"></th> </tr> </thead> <tbody> <tr> <td style="text-align: center;">FFP1</td> <td style="text-align: center;">0.6</td> <td style="text-align: center;">2.1</td> <td style="text-align: center;">3.0</td> <td colspan="2"></td> </tr> <tr> <td style="text-align: center;">FFP2</td> <td style="text-align: center;">0.7</td> <td style="text-align: center;">2.4</td> <td style="text-align: center;">3.0</td> <td colspan="2"></td> </tr> <tr> <td style="text-align: center;">FFP3</td> <td style="text-align: center;">1.0</td> <td style="text-align: center;">3.0</td> <td style="text-align: center;">3.0</td> <td colspan="2"></td> </tr> </tbody> </table> | | | | | | | | | | | Classification | Maximum permitted resistance (mbar) | | | | | Inhalation | | | Exhalation | | 30 l/min | 95 l/min | 160 l/min | | | FFP1 | 0.6 | 2.1 | 3.0 | | | FFP2 | 0.7 | 2.4 | 3.0 | | | FFP3 | 1.0 | 3.0 | 3.0 | | |
| Classification | Maximum permitted resistance (mbar) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Inhalation | | | Exhalation | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | 30 l/min | 95 l/min | 160 l/min | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| FFP1 | 0.6 | 2.1 | 3.0 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| FFP2 | 0.7 | 2.4 | 3.0 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| FFP3 | 1.0 | 3.0 | 3.0 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

Appendix 5: Summarization of Test DataBreathing resistance (mbar)

| | Flow rate(l/min) | | 1 | | | | | 2 | | | | | 3 | | | | |
|-----------------------------|------------------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| | | | A | B | C | D | E | A | B | C | D | E | A | B | C | D | E |
| As received | Inhalation | 30 | 0.2 | 0.2 | 0.2 | 0.2 | 0.3 | 0.3 | 0.3 | 0.2 | 0.2 | 0.2 | 0.2 | 0.2 | 0.2 | 0.3 | 0.2 |
| | | 95 | 0.8 | 0.7 | 0.8 | 0.8 | 0.8 | 0.7 | 0.8 | 0.8 | 0.8 | 0.8 | 0.7 | 0.8 | 0.9 | 0.8 | 0.8 |
| | Exhalation | 160 | 1.5 | 1.6 | 1.5 | 1.6 | 1.7 | 1.6 | 1.6 | 1.6 | 1.6 | 1.5 | 1.6 | 1.6 | 1.6 | 1.6 | 1.7 |
| Simulated wearing treatment | Flow rate(l/min) | | 4 | | | | | 5 | | | | | 6 | | | | |
| | Inhalation | 30 | 0.3 | 0.3 | 0.2 | 0.2 | 0.3 | 0.3 | 0.2 | 0.3 | 0.3 | 0.3 | 0.2 | 0.3 | 0.2 | 0.3 | 0.3 |
| | | 95 | 0.9 | 0.8 | 0.8 | 0.7 | 0.8 | 0.8 | 0.8 | 0.9 | 0.8 | 0.8 | 0.9 | 0.7 | 0.8 | 0.8 | 0.9 |
| | Exhalation | 160 | 1.6 | 1.6 | 1.4 | 1.5 | 1.6 | 1.6 | 1.5 | 1.5 | 1.4 | 1.6 | 1.6 | 1.6 | 1.6 | 1.5 | 1.5 |
| Temperature conditioned | Flow rate(l/min) | | 7 | | | | | 8 | | | | | 9 | | | | |
| | Inhalation | 30 | 0.2 | 0.2 | 0.2 | 0.3 | 0.2 | 0.2 | 0.2 | 0.3 | 0.2 | 0.2 | 0.2 | 0.2 | 0.2 | 0.3 | 0.2 |
| | | 95 | 0.7 | 0.7 | 0.6 | 0.7 | 0.7 | 0.6 | 0.6 | 0.7 | 0.6 | 0.6 | 0.6 | 0.6 | 0.6 | 0.7 | 0.7 |
| | Exhalation | 160 | 1.3 | 1.3 | 1.4 | 1.3 | 1.4 | 1.3 | 1.3 | 1.3 | 1.4 | 1.3 | 1.3 | 1.4 | 1.4 | 1.3 | 1.4 |

A: facing directly ahead; B: facing vertically upwards; C: facing vertically downwards; D: lying on the left side; E: lying on the right side

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions. If any, The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone : (86-21) 54966703, or email: CN.Goccheck@sgs.com



3 Building, No.889, Yuhai Road, Xuhui District, Shanghai, China: 200233
 中国·上海·徐汇区宜山路889号3号楼 邮编: 200233

1 (86-21) 61402888 1 (86-21) 61402886 1 (86-21) 64966703 1 (86-21) 64966703
www.sgsgroup.com sps.china@sgs.com

Clause 7.17 Clogging

(EN 149:2001+A1:2009, Clause 8.9 & 8.10)

| Test Requirement | | Results | Comment |
|---|--|---------------------------------------|---------|
| <u>Clause 7.17.2 Breathing resistance</u> Valved particle filtering half masks: After clogging the inhalation resistances shall not exceed: FFP1: 4 mbar, FFP2: 5 mbar, FFP3: 7 mbar at 95L/min continuous flow The exhalation resistance shall not exceed 3 mbar at 160 L/min continuous flow. | | Optional for single shift device only | N.A. |
| Valveless particle filtering half masks: After clogging the inhalation and exhalation resistances shall not exceed: FFP1: 3 mbar, FFP2: 4 mbar, FFP3: 5 mbar at 95L/min continuous flow | | | |
| <u>Clause 7.17.3 Penetration of filter material</u> All types (valved and valveless) of particle filtering half masks claimed to meet the clogging requirement shall also meet the requirements. | | | |

| Classification | Maximum penetration of test aerosol | |
|----------------|-------------------------------------|----------------------------|
| | Sodium chloride test 95 l/min | Paraffin oil test 95 l/min |
| | % | % |
| max. | | max. |
| FFP1 | 20 | 20 |
| FFP2 | 6 | 6 |
| FFP3 | 1 | 1 |

Clause 7.18 Demountable Parts

(EN 149:2001+A1:2009, Clause 8.2)

| Test Requirement | | Results | Comment |
|--|--|----------------------|---------|
| All demountable parts (if fitted) shall be readily connected and secured, where possible by hand | | No demountable parts | N.A. |

| Test | Uncertainty |
|--|-------------|
| Total inward leakage | 3.4% |
| Penetration of filter material | 4.8% |
| Carbon dioxide content of the inhalation air | 3.9% |
| Breathing resistance (30L/min) | 5.9% |
| Breathing resistance (95L/min) | 4.9% |
| Breathing resistance (160L/min) | 4.3% |

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.


Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone: (021) 54967143, or email: CN.Goccheck@sgs.com



3 Building No.889, Yuhai Road, Xuhui District Shanghai, China: 200233
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233

1 (86-21) 61402888 1 (86-21) 64966703 www.sgsgroup.com
1 (86-21) 61402888 1 (86-21) 64966703 sgschina@sgs.com

Sample Photo

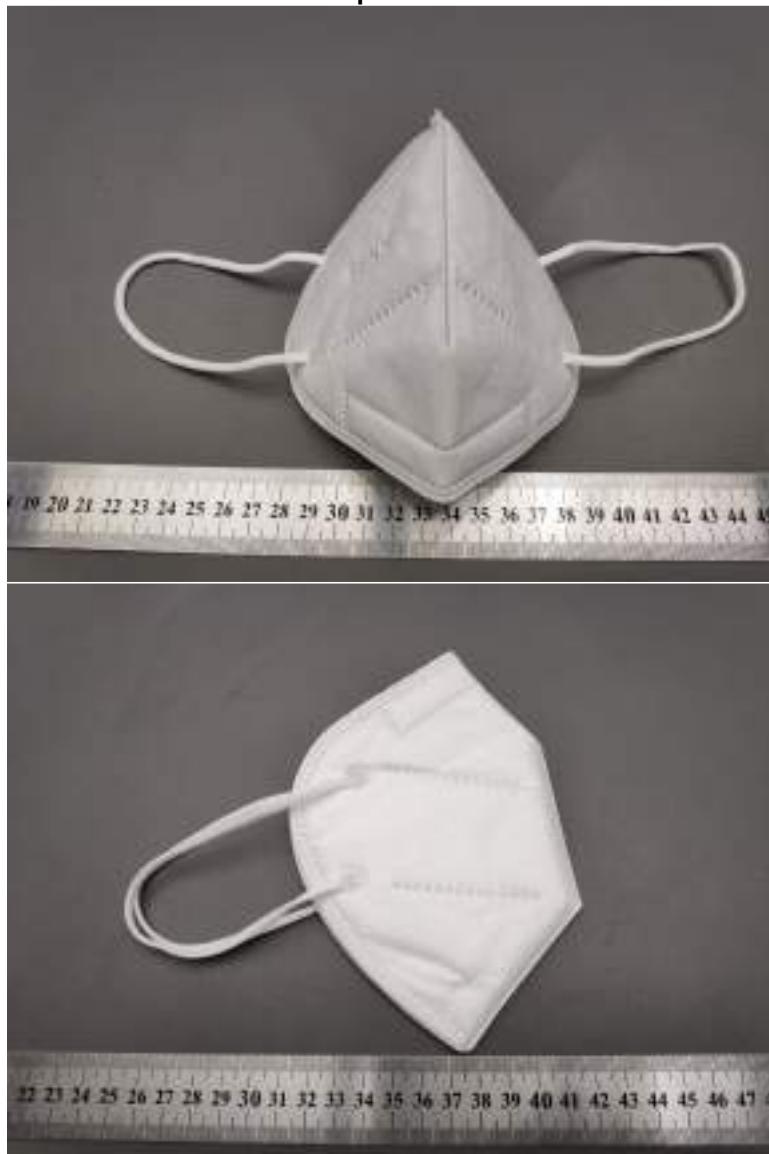

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone : (86-788) 81871443, or email: CN.Goccheck@sgs.com



SGS China Testing Center
Shanghai, China

3rd Building, No.889, Yuhai Road, Xuhui District, Shanghai, China: 200233
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233

T: (86-21) 61402888 F: (86-21) 64998703
www.sgsgroup.com.cn
sgschina@sgs.com



End of Report

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone : (86-788) 81871443, or email: CN.Goccheck@sgs.com



SGS China Testing Center
Shanghai

3rd Building, No.889, Yuhai Road, Xuhui District, Shanghai, China: 200233
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233

T: (86-21) 61402888 F: (86-21) 64966703
www.sgsgroup.com.cn
E: sgschina@sgs.com